

Startrol LED Ceiling Mount Exam Light Schematic

Item No. CSLED-C

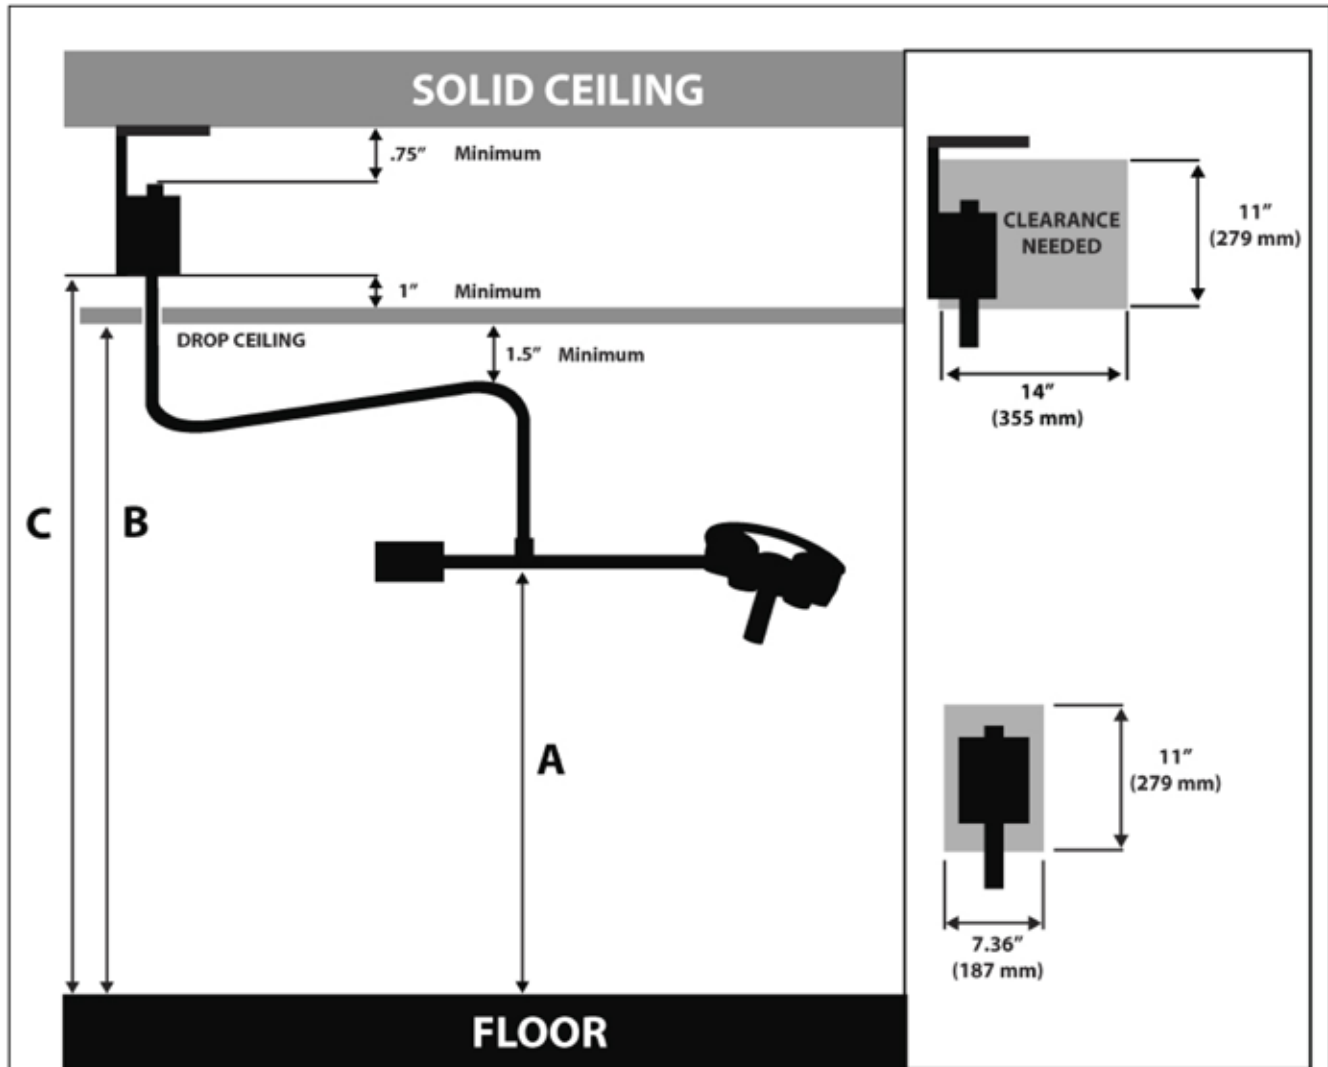


Figure 6.1.2 Minimum Clearances

To Achieve Floor to Light Distance of "A"	If Drop Ceiling is "B"	Mount bottom of Power Supply Housing From Floor At "C"
63 inches (1600 mm)	7.5 feet (2280 mm)	98 inches (2489 mm)
63 inches (1600 mm)	8.0 feet (2440 mm)	98 inches (2489 mm)
68 inches (1600 mm)	8.0 feet (2440 mm)	103 inches (2616 mm)
75 inches (1727 mm)	9.0 feet (2740 mm)	110 inches (2794 mm)

api
anthony products, inc.